



Your environment. Our sensor network.

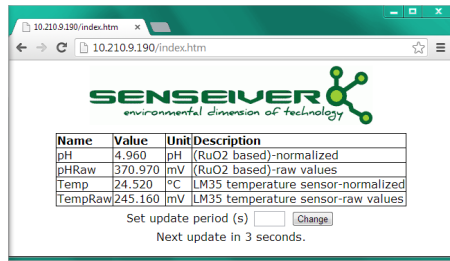




Name	Value	Unit	Description
pH	4.960	pH	(RuO2 based)-normalized
pHRaw	370.970	mV	(RuO2 based)-raw values
Temp	24.520	°C	LM35 temperature sensor-normalized
TempRaw	245.160	mV	LM35 temperature sensor-raw values

Set update period (s) Change
Next update in 3 seconds.

Visualization

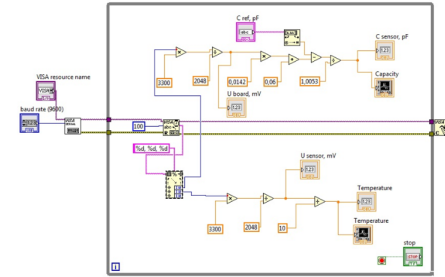

Software

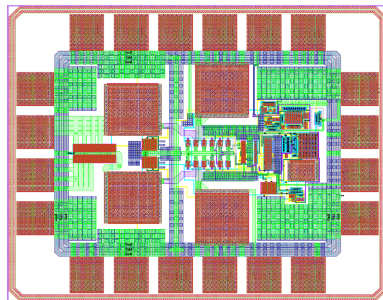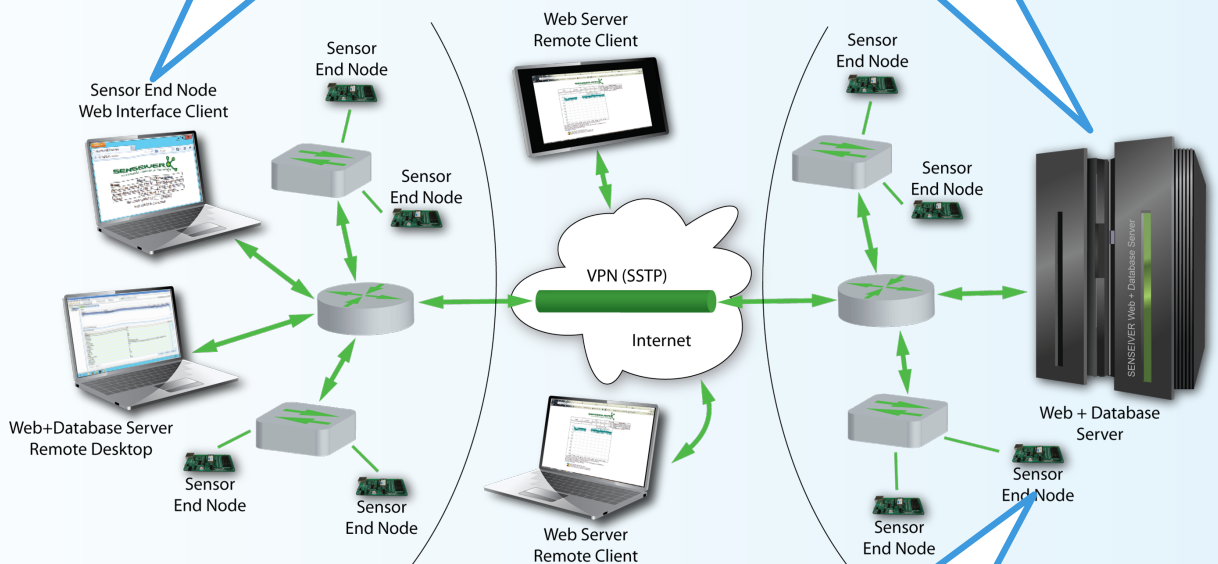

Communication



Hardware



Sensors



dr inż. Piotr Guzdek
Institute of Electron Technology
Division in Kraków
ul. Zabłocie 39
30-701 Kraków
tel.: 12 656 3144
e-mail: pguzdek@ite.waw.pl

Visit our website: www.centrum-itcc.ite.waw.pl or www.senseiver.com.